




Datum 09-04-19	Start 09:28:48	Stopp 09:47:33	S/N ST01-00260
Programm 134	Prozessnummer 00009		Firmware 27.3

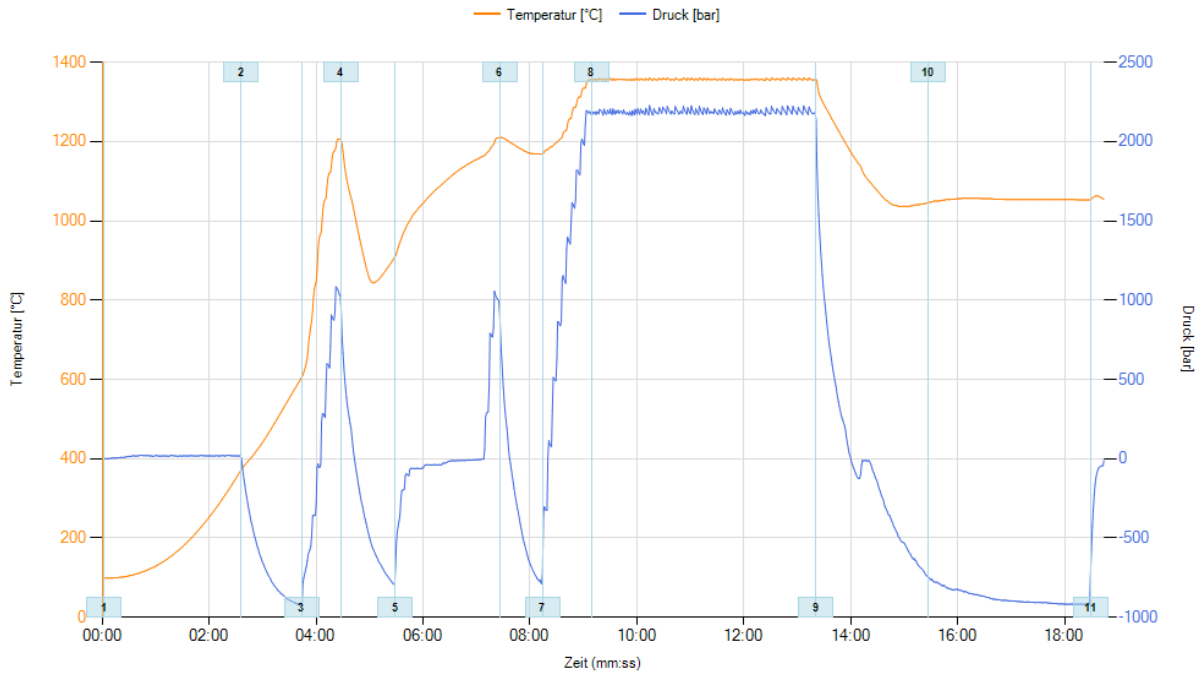

Phase	Zeit [mm:ss]	Schritt [mm:ss]	p [bar]	t [°C]	t calc. [°C]
0 Locking door	00:01		0.002	9.9	9.9
1 Heating up	00:02	02:33	0.019	36.9	36.9
2 Vacuum I	02:36	01:07	-0.925	60.3	60.3
3 Steam Pulse I	03:44	00:43	1.031	120.5	120.5
4 Vacuum II	04:28	01:00	-0.795	90.8	90.8
5 Steam Pulse II	05:29	01:56	0.996	121.0	121.0
6 Vacuum III	07:26	00:47	-0.789	116.9	116.9
7 Pressurizing	08:14	00:54	2.174	135.7	135.7
8 Sterilizing	09:09	04:11	2.175	135.7	135.6
9 Depressurizing	13:21	02:05	-0.740	104.5	104.5
10 Drying	15:27	03:01	-0.918	105.3	105.3
11 Equalizing	18:29	00:14	-0.043	105.6	105.6
12 Ulocking door	18:44		-0.011	105.5	105.5

Sterilization Complete

Sterilisationstemper 134

Zeit 04:11

Min. Temperatur 135,6

Max. Temperatur 136

Min. Druck 2,16

Max. Druck 2,23

Teststerilisation bei Lieferung
 Inhalt: unverpackt
 Gelenkzange
 Pinzette
 Tamponierer

Label